



Access this article online

Quick Response Code:



Website:

www.turkjemergmed.com

DOI:

10.4103/2452-2473.348436

Comparison of endotracheal intubation with Macintosh versus King Vision video laryngoscope using coronavirus disease 2019 barrier box on manikins: A randomized crossover study

Satyabrata Guru¹, Neha Singh², Sangeeta Sahoo^{1*}, Upendra Hansda¹, Chittaranjan Mohanty¹

Departments of ¹Trauma and Emergency and ²Anaesthesiology, AIIMS, Bhubaneswar, Odisha, India

*Corresponding author

Abstract:

BACKGROUND: Coronavirus disease 2019 (COVID-19) virus usually spreads through aerosol and close contact. Frontline health-care workers handle aerosol-generating procedures like endotracheal intubation. To reduce this risk, COVID-19 barrier box came into the picture. However, the COVID-19 barrier box may compromise easy and successful intubation, and their limitation must be studied.

OBJECTIVES: The objective of this study was to assess the time to successful intubation with or without the COVID-19 barrier box using the Macintosh laryngoscope and King Vision video laryngoscope (KVVL). We also assessed the first-pass success rate, ease of intubation, Cormack–Lehane (CL) grade, and requirement of external laryngeal manipulation.

METHODS: We conducted this manikin-based randomized crossover study to assess the time to successful intubation by anesthesiologists (22) and emergency physicians (11) having 1 year or more experience with or without COVID-19 barrier box by using the Macintosh laryngoscope and KVVL. Our study randomized the sequence of the four different intubation scenarios.

RESULTS: The comparison of mean duration of intubation between KVVL (13.21 ± 4.05 s) and Macintosh laryngoscope (12.89 ± 4.28 s) with COVID-19 barrier box was not statistically significant (95% confidence interval: 1.21–0.97). The ease of intubation, number of attempts, and requirement of external laryngeal manipulation were not statistically significant. Intubations were statistically significant more difficult with barrier box in view of higher CL grade.

CONCLUSION: Time to intubation was longer with COVID-19 barrier box using KVVL as compared to Macintosh laryngoscope which was statistically not significant.

Keywords:

Coronavirus disease 2019, intubation, King Vision video laryngoscope, Macintosh laryngoscope, manikin

Submitted: 04-02-2022
Revised 1: 16-03-2022
Revised 2: 13-04-2022
Revised 3: 06-05-2022
Accepted: 17-05-2022
Published: 01-07-2022

ORCID:

SG: 0000000245475323
NS: 0000-0003-2013-4295
SS: 0000-0003-2836-6357
UH: 0000-0002-5703-4135
CM: 0000-0002-8525-2084

Address for correspondence:

Dr. Sangeeta Sahoo,
Department of Trauma
and Emergency, Room
No. 342, 3rd Floor,
Academic Block, AIIMS,
Bhubaneswar, Odisha,
India.
E-mail: drsangeeta.asth@gmail.com

Introduction

Coronavirus disease 2019 (COVID-19) was declared as pandemic by the WHO on March 11, 2020. The causative organism

This is an open access journal, and articles are distributed under the terms of the Creative Commons Attribution-NonCommercial-ShareAlike 4.0 License, which allows others to remix, tweak, and build upon the work non-commercially, as long as appropriate credit is given and the new creations are licensed under the identical terms.

For reprints contact: WKHLRPMedknow_reprints@wolterskluwer.com

of the disease (severe acute respiratory syndrome-coronavirus-2) usually spreads through droplets and aerosols. Various aerosol-generating procedures such as endotracheal intubation and bag-mask ventilation are being performed by frontline

How to cite this article: Guru S, Singh N, Sahoo S, Hansda U, Mohanty C. Comparison of endotracheal intubation with Macintosh versus King Vision video laryngoscope using coronavirus disease 2019 barrier box on manikins: A randomized crossover study. *Turk J Emerg Med* 2022;22:149-55.

Box-ED section

What is already known on the study topic?

- Coronavirus disease 2019 (COVID-19) is very contagious and spreads through aerosol. The highest viral load of severe acute respiratory syndrome-coronavirus-2 appears in sputum and upper airway secretions. Frontline health-care workers performing various aerosol-generating procedures such as endotracheal intubation are at risk. This COVID-19 barrier box has proven to reduce the aerosol spread during endotracheal intubation.

What is the conflict on the issue? Has it important for readers?

- Macintosh laryngoscope is commonly used laryngoscope in the emergency department. The King Vision video laryngoscope (KVVV) is a portable, inexpensive, and suitable for use in the emergency department. Using these laryngoscopes with the COVID-19 barrier box may compromise easy and successful intubation, and their limitation must be studied.

How is this study structured?

- Our study is a manikin-based randomized crossover study to assess the time to successful intubation by the emergency physicians and anesthesiologists having 1 year or more experience with or without COVID-19 barrier box by using the Macintosh laryngoscope and KVVV.

What does this study tell us?

- Both Macintosh laryngoscope and KVVV can be used for intubation with COVID-19 barrier.

health-care workers.^[1] The COVID-19 pandemic is continuing and creating serious challenges to the health-care personnel involved in airway management. Various tools have been invented to curtail this risk to the person managing the airway, like the aerosol box.^[2] The COVID-19 barrier box covers the patient's head and neck and effectively reduces the aerosol spread during endotracheal intubation.^[3-5] Further, the COVID-19 barrier box without negative pressure may increase the risk to patients and health-care providers.^[6-9]

Although the need for a change in intubation practice through barriers to reduce the aerosol spread is apparent, it will not be without a learning curve. The Macintosh laryngoscope is used commonly in the emergency department, intensive care units, and operation theater. The King Vision video laryngoscope (KVVV) (AMBU, Denmark) is another portable, inexpensive, and suitable option for the emergency department. Using these laryngoscopes with the aerosol box may compromise easy and

successful intubation. Therefore, their limitations or benefits must be studied.

We conducted this manikin-based study to assess the time to successful intubation by anesthesiologists and emergency physicians having 1 year or more experience with or without aerosol box using the Macintosh laryngoscope and KVVV. We also assessed the first-pass success rate, ease of intubation, Cormack-Lehane (CL) grade, and requirement of external laryngeal manipulation.

Methods

Study type

This study was a manikin-based randomized crossover study. After getting approval from the Institute Ethics committee (IEC NO-T/IM-NF/TandEM/20/39 dated November 12, 2020), it was registered in the Clinical Trials Registry-India (CTRI/2021/02/031052).

Study population

Participants were the faculty members and residents of the anesthesia and emergency medicine departments who had experience of intubation for more than 1 year and familiar with using both KVVV and Macintosh laryngoscope. Participant refusal was taken as exclusion criteria. Written informed consent was obtained from each participant before the study.

Study design

The participants practiced intubation 20 times on manikin with COVID-19 barrier box: 10 times using Macintosh laryngoscope and 10 times using KVVV after demonstration by the investigators (SS, UH, CM, NS, and SD). The intubation was done in a simulated environment. The Airway Trainer Manikin (Laerdal Medical, Stavanger, Norway) was used for practice and study. The COVID-19 barrier box used was a modified version of the basic model by Sahoo *et al.*^[10,11] [Figure 1]. In the basic model, visualization of the vocal cord was not proper due to the right-angle joint. Hence, the height of the vertical wall and the length of the horizontal roof were decreased, and an additional slanting roof was made, which improved the visualization of the vocal cord. Moreover, the creation of side opening helped in providing backward-upward-rightward pressure, suction, and bougie. All the participants were acquainted with the COVID-19 barrier box before doing the study. All intubations were done using either a size 3 Macintosh blade or channeled version of the KVVV blade, with a cuffed 7.5-mm internal diameter endotracheal tube (Smiths Medical, St. Paul, MN, USA). The lubricant was used with both the blade and the endotracheal tube while using the KVVV. An investigator was there to help with the equipment or external laryngeal manipulation

The median years of experience was 4 years (IQR [25th-75th percentile]: 2.25-7) [Table 1].

The comparison of mean duration of intubation using Macintosh blade with (12.89 ± 4.28 s) and without (11.82 ± 4.25 s) COVID-19 barrier box was not statistically significant (95% CI: 0.04-2.18) [Table 2]. The comparison of mean duration of intubation with KVVl laryngoscope with (13.21 ± 4.05 s) and without (12.08 ± 3.73 s) COVID-19 barrier box was not statistically significant (95% CI: 0.47-1.85) [Table 3]. Similarly, we did not find any statistically significant difference between the Macintosh

laryngoscope and KVVl with barrier box (95% CI: 1.21-0.97) [Table 4]. Ease of intubation, number of attempts, and requirement of external laryngeal manipulation were not statistically significant with or without the COVID-19 barrier box. Second intubation attempts were required three times each for both the laryngoscopes with barrier box. There was a statistically significant higher CL grade (CL Grade 2) in case of Macintosh laryngoscope compared to KVVl with COVID-19 barrier box (95% CI: 0.06-0.52). There was a significant correlation between the duration of intubation with Macintosh laryngoscope and the years of experience ($r = -0.420$), but weak correlation between the duration of intubation with KVVl and years of experience ($r = -0.146$) [Figure 4].

Table 1: Demographic characteristics of the study participants

Variables	Median IQR (25 th -75 th percentile) or n (%)
Age (years)	30 (28.0-35.5)
Gender	
Male	26 (78.8)
Female	7 (21.2)
Designation	
Faculty	9 (27.3)
Resident	24 (21.2)
Department	
Anesthesia specialist	22 (67.6)
Emergency specialist	11 (32.4)
Years of experiences	4 (2.25-7.0)

IQR: Interquartile range

Discussion

We did not find any significant difference in the intubation time with the Macintosh laryngoscope blade and KVVl with or without the COVID-19 barrier box. With the COVID-19 barrier box, the average duration of intubation using KVVl was 13.21 ± 4.05 s, whereas the duration was 12.89 ± 4.28 s with the Macintosh laryngoscope. Intubations were statistically significant more difficult with barrier box in view of higher CL grade.

The duration of intubation was more with Macintosh laryngoscope using COVID barrier box in participants

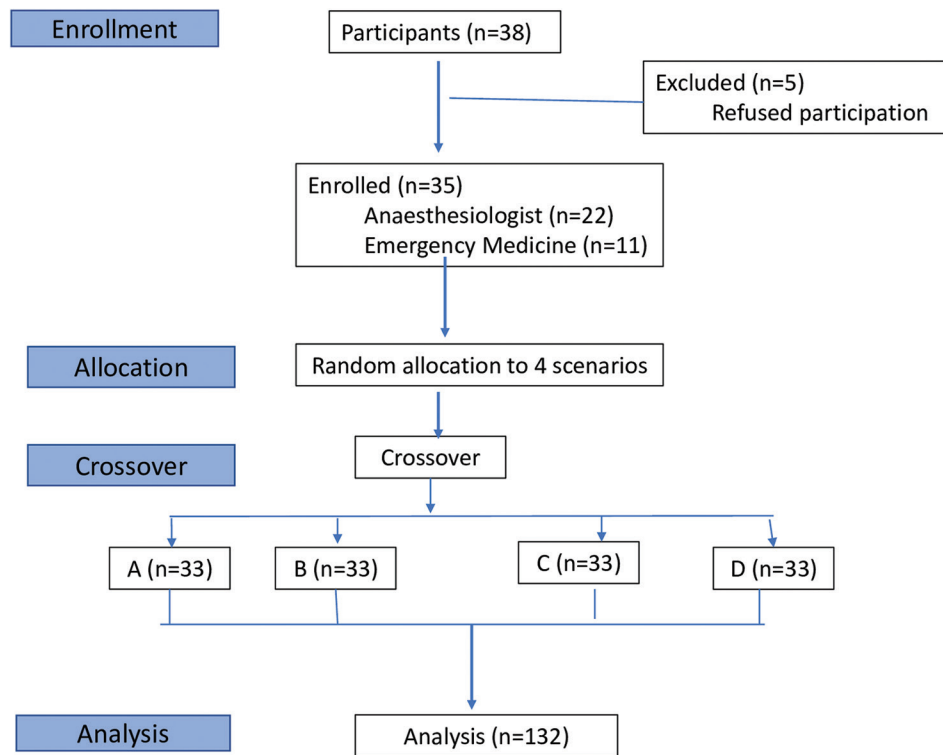


Figure 3: Consort flowchart of study participants. (a) Intubation with Macintosh laryngoscope without COVID barrier box group, (b) Intubation with Macintosh laryngoscope with COVID barrier box group, (c) Intubation with KVVl without COVID barrier box, (d) Intubation with KVVl with COVID barrier box group. COVID-19: Coronavirus disease 2019, KVVl: King Vision video laryngoscope

Table 2: Comparison of different parameters for Macintosh laryngoscope with or without coronavirus disease barrier box

Variables	With COVID barrier box, n (%)	Without COVID barrier box, n (%)	Mean difference/OR (95% CI)
Duration (s), mean±SD	12.89±4.28	11.82±4.25	1.07 (-0.04-2.18)
Ease of intubation			
Grade I	7 (21.2)	11 (33.3)	1 (reference)
Grade II	18 (54.5)	18 (54.5)	0.64 (0.20-2.01)
Grade III	5 (15.2)	3 (9.1)	0.38 (0.07-2.12)
Grade IV	3 (9.1)	1 (3.0)	0.21 (0.02-2.46)
CL grade			
Grade 1	14 (42.4)	13 (39.4)	1 (reference)
Grade 2	19 (57.6)	20 (60.6)	1.13 (0.43-3.03)
Number of attempts			
1	31 (93.9)	33 (100.0)	Reference
>1	2 (6.1)	0	-
ELM			
No	32 (97.0)	33 (100.0)	Reference
Yes	1 (3.0)	0	-

*95% CI for duration was calculated for mean difference. CI for number of attempts and ELM could not be calculated. CI: Confidence interval, ELM: External laryngeal manipulation, SD: Standard deviation, OR: Odds ratio, CL: Cormack-Lehane, COVID: Coronavirus disease

Table 3: Comparison of different parameters for video laryngoscope with or without coronavirus disease barrier box

Variables	With COVID barrier box, n (%)	Without COVID barrier box, n (%)	Mean difference/OR (95% CI)*
Duration (s), mean±SD	13.21±4.05	12.08±3.73	1.13 (-0.47-1.85)
Ease of intubation			
Grade I	7 (21.2)	7 (21.2)	Reference
Grade II	19 (57.6)	19 (57.6)	0.98 (0.29-3.41)
Grade III	6 (18.2)	6 (18.2)	0.97 (0.21-4.67)
Grade IV	1 (3.0)	1 (3.0)	0.99 (0.05-19.4)
CL grade			
Grade 1	27 (81.8)	27 (81.8)	Reference
Grade 2	6 (18.2)	6 (18.2)	0.97 (0.29-3.49)
Number of attempts			
1	32 (97.0)	33 (100.0)	Reference
>1	1 (3.0)	0	-
ELM			
No	32 (97.0)	32 (97.0)	Reference
Yes	1 (3.0)	1 (3.0)	0.99 (0.06-16.69)

*95% CI for duration was calculated for difference in mean. CI for number of attempts could not be calculated. CI: Confidence interval, ELM: External laryngeal manipulation, SD: Standard deviation, OR: Odds ratio, CL: Cormack-Lehane, COVID: Coronavirus disease

having less year of experience, but the year of experience had no correlation with KVV L.

Fong *et al.*, in their randomized crossover manikin-based simulation study using the aerosol box with GlideScope, found that the aerosol box increased the intubation time by 6 s which was not statistically significant.^[13] They

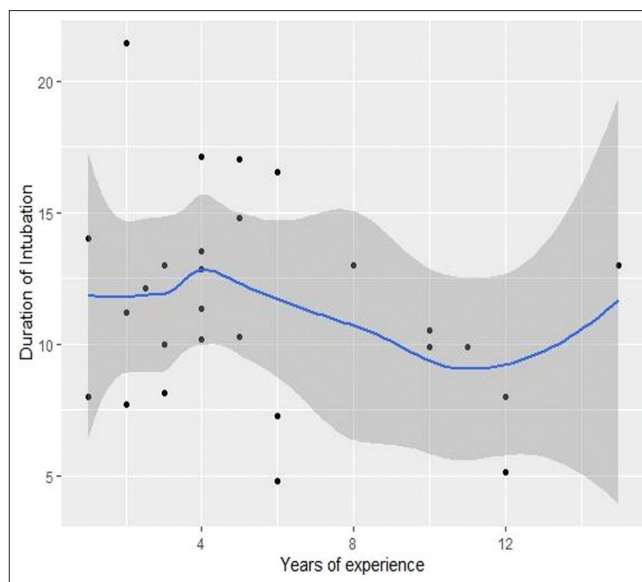


Figure 4: Correlation between duration of intubation with Macintosh laryngoscope and years of experience

also reported that the aerosol box could be an adjunct to personal protective equipment (PPE) to reduce the aerosol spread. Our study found that COVID-19 barrier box increased intubation time in both Macintosh laryngoscope and KVV L, but it was not statistically significant.

Kannaujia *et al.* had done a simulation study on manikin found no significant difference in intubation time, glottic view, and the first-pass success rate with or without the aerosol box using GlideScope video laryngoscope, which was similar to our study.^[14] However, the participants included in their study were senior consultant anesthesiologists, while we included both residents and consultants of both anesthesia and emergency departments, which is more generalizable.

Abolkheir *et al.* had done a manikin study, found time to intubation was more with GlideScope than Macintosh laryngoscope which was similar to our study.^[15]

Our study also got similar findings to a few other studies conducted in real patients with COVID-negative status. The barrier box did not cause delay in intubation time in a non-inferiority trial comparing with and without barrier box.^[16] In prospective trials by Jen *et al.* and Sahoo *et al.* in COVID-19-negative patients with normal airways, the use of the COVID-19 barrier box did not significantly delay the intubation time nor decrease the first-pass success rate.^[17,18]

During this COVID era, the role of PPE was crucial for health-care providers' safety.^[19] Shortage of PPE was also seen in a few places because of its extensive use during patient care. The idea of improving safety leads to the development of the barrier box.

Table 4: Comparison of different parameters for Macintosh and video laryngoscope with coronavirus disease barrier box

	Macintosh laryngoscope with COVID barrier box, n (%)	Video laryngoscope with COVID barrier box, n (%)	Mean difference/ OR (95% CI)*
Duration (s), mean±SD	12.89±4.28	13.21±4.05	-0.32 (-1.21-0.97)
Ease of intubation			
Grade I	7 (21.2)	7 (21.2)	Reference
Grade II	18 (54.5)	19 (57.6)	1.0 (0.29-3.43)
Grade III	5 (15.2)	6 (18.2)	1.2 (0.25-5.84)
Grade IV	3 (9.1)	1 (3.0)	0.33 (0.03-4.04)
CL grade			
Grade 1	14 (42.4)	27 (81.8)	Reference
Grade 2	19 (57.6)	6 (18.2)	0.17 (0.06-0.52)
Number of attempts			
1	31 (93.9)	32 (97.0)	Reference
>1	2 (6.1)	1 (3.0)	0.50 (0.04-5.80)
ELM			
No	32 (97.0)	32 (97.0)	Reference
Yes	1 (3.0)	1 (3.0)	0.97 (0.06-16.18)

*95% CI for duration was calculated for difference in mean. . CI: Confidence interval, ELM: External laryngeal manipulation, SD: Standard deviation, OR: Odds ratio, CL: Cormack-Lehane, COVID: Coronavirus disease

Limitations

Unlike Begley *et al.*, we have not studied the PPE breach in our manikin study due to resource constraints.^[20] We have not studied the difficult airway scenarios and the degree of aerosol spread in our study. As the study has been done in simulated environment, the results may differ in clinical scenario. However, our findings are similar to few clinical studies. All the participants have more than 1 year of experience, and findings may be different when used by novice residents during airway management. We have not studied the effect of other types of protective barriers such as hoods and tents. The results from this study may not be generalizable to other design of COVID-19 barrier box.

Conclusion

The time to intubation was more with the COVID-19 barrier box using with KVV L than Macintosh laryngoscope which was not statistically significant. Hence, both Macintosh laryngoscope and KVV L can be used for intubation with a COVID barrier box. Further randomized control trials with a larger sample size may be considered in COVID-19-positive patients to validate these data with a barrier box.

Acknowledgment

We would like to thank the Council of Scientific and Industrial Research-Institute of Minerals and Materials Technology, Bhubaneswar, for designing the COVID barrier box.

Author contributions

SS: conceptualization; data curation; formal analysis; methodology; project administration; resources; supervision; validation; writing – review and editing. NS: data curation; investigation; methodology; visualization; writing – original draft: data curation; investigation; visualization; writing – original draft; writing – review and editing. UH: data curation; visualization; writing – original draft; writing – review and editing. CM: methodology; data curation; investigation; visualization; writing – original draft; writing – review and editing. SG: methodology; data curation; investigation; visualization; writing – original draft; writing – review and editing.

Conflicts of interest

None Declared.

Ethical approval

This protocol was approved by the Ethics Committee of AIIMS, Bhubaneswar, Odisha, India, IEC NO-T/IM-NF/T&EM/20/39 dated November 12, 2020.

Funding

None.

References

- Cook TM, El-Boghdady K, McGuire B, McNarry AF, Patel A, Higgs A. Consensus guidelines for managing the airway in patients with COVID-19: Guidelines from the Difficult Airway Society, the Association of Anaesthetists the Intensive Care Society, the Faculty of Intensive Care Medicine and the Royal College of Anaesthetists. *Anaesthesia* 2020;75:785-99.
- Canelli R, Connor CW, Gonzalez M, Nozari A, Ortega R. Barrier enclosure during endotracheal intubation. *N Engl J Med* 2020;382:1957-8.
- Van Zundert TC, Barach P, Van Zundert AA. Revisiting safe airway management and patient care by anaesthetists during the COVID-19 pandemic. *Br J Anaesth* 2020;125:863-7.
- Ibrahim M, Khan E, Babazade R, Simon M, Vadhera R. Comparison of the effectiveness of different barrier enclosure techniques in protection of healthcare workers during tracheal intubation and extubation. *A A Pract* 2020;14:e01252.
- Dhillon RS, Rowin WA, Humphries RS, Kevin K, Ward JD, Phan TD, *et al.* Aerosolisation during tracheal intubation and extubation in an operating theatre setting. *Anaesthesia* 2021;76:182-8.
- The U.S. Food and Drug Administration. Protective Barrier Enclosures Without Negative Pressure Used During the COVID-19 Pandemic May Increase Risk to Patients and Health Care Providers-Letter to Health Care Providers. U.S. Food Drug Administration; 2020.
- Singh N, Ponde VC, Sahoo S, Mohanty CR. Improving the efficacy of the plastic tents and boxes used for airway management of coronavirus disease-19 patients: Seal and negative suction. *Minerva Anesthesiol* 2020;86:1252-3.
- Singh N, Ponde VC, Sahoo S, Mohanty CR. Barrier enclosure systems use in COVID-19 along with sealing and suction: Something is better than nothing. *Minerva Anesthesiol* 2021;87:377-8.
- Simpson JP, Wong DN, Verco L, Carter R, Dzidowski M, Chan PY. Measurement of airborne particle exposure during simulated tracheal intubation using various proposed aerosol containment devices during the COVID-19 pandemic. *Anaesthesia* 2020;75:1587-95.
- Everington K. Taiwanese Doctor Invents Device to Protect US Doctors Against Coronavirus. *Taiwan News*; 2020. Available from: <https://www.taiwannews.com.tw/en/news/3902435>. [Last accessed on 2022 Feb 03].

Guru, et al.: Macintosh versus KVVV for intubation on manikins

11. Sahoo S, Hansda U, Mohanty CR, Mishra N. Modified aerosol box for endotracheal intubation: A safeguard for the frontline healthcare workers during COVID pandemic. *J Family Med Prim Care* 2020;9:5802-3.
12. Park SO, Shin DH, Lee KR, Hong DY, Kim EJ, Baek KJ. Efficacy of the Disposcope endoscope, a new video laryngoscope, for endotracheal intubation in patients with cervical spine immobilisation by semirigid neck collar: Comparison with the Macintosh laryngoscope using a simulation study on a manikin. *Emerg Med J* 2013;30:270-4.
13. Fong S, Li E, Violato E, Reid A, Gu Y. Impact of aerosol box on intubation during COVID-19: A simulation study of normal and difficult airways. *Can J Anaesth* 2021;68:496-504.
14. Kannaujia A, Haldar R, Shamim R, Mishra P, Agarwal A. Comparative evaluation of intubation performances using two different barrier devices used in the COVID-19 era: A manikin based pilot study. *Saudi J Anaesth* 2021;15:86-92.
15. Abolkheir AB, El-Kabbani A, Al Raffa A, AlFattani A, Norris A. Comparative performance of two protective barriers during tracheal intubation of COVID-19 patients: A simulation cross-over study. *Saudi J Anaesth* 2021;15:396-402.
16. Madabhushi P, Kinthala S, Ankam A, Chopra N, Porter BR. Time to adapt in the pandemic era: A prospective randomized non-inferiority study comparing time to intubate with and without the barrier box. *BMC Anesthesiol* 2020;20:232.
17. Jen TT, Gusti V, Badh C, Mehta S, Denomme J, Lockhart S, et al. The impact of a barrier enclosure on time to tracheal intubation: A randomized controlled trial. *Can J Anaesth* 2021;68:1358-67.
18. Sahoo S, Singh N, Mohanty CR, Hansda U, Sahoo J, Sahu A. Macintosh laryngoscope versus AMBU King Vision video laryngoscope for endotracheal intubation using a COVID-19 barrier box: A randomized controlled trial. *Int J Crit Illn Inj Sci* 2021;11:151-5.
19. Lockhart SL, Duggan LV, Wax RS, Saad S, Grocott HP. Personal protective equipment (PPE) for both anesthesiologists and other airway managers: Principles and practice during the COVID-19 pandemic. *Can J Anaesth* 2020;67:1005-15.
20. Begley JL, Lavery KE, Nickson CP, Brewster DJ. The aerosol box for intubation in coronavirus disease 2019 patients: An *in-situ* simulation crossover study. *Anaesthesia* 2020;75:1014-21.